

Failure Patterns of Severely Compromised Endodontically Treated Anterior Teeth: A Comparative *In Vitro* Study of Two Restorative Approaches



Abed Alhade Kheder^{1,*} , Rima Jawdat Saker¹ and Ziad Albash² 

¹Fixed Prosthodontics, Tishreen University, Latakia, Syrian Arab Republic

²Department Oral and Maxillofacial Surgery, Tishreen University, Latakia, Syrian Arab Republic

Abstract:

Introduction: This *in vitro* study aimed to compare the failure patterns of two restorative techniques in severely damaged, endodontically treated maxillary central incisors: (1) endocrowns fabricated from lithium disilicate ceramic (IPS e.max Press), and (2) quartz-fiber posts with composite resin cores and lithium disilicate crowns (IPS e.max Press).

Materials and Methods: Twenty freshly extracted human maxillary central incisors with intact roots, comparable in length, morphology, and size, were selected. The teeth were randomly allocated into two groups (n = 10): Group I, restored with lithium disilicate endocrowns (IPS e.max Press), and Group II, restored with quartz-fiber posts, composite resin cores, and lithium disilicate crowns (IPS e.max Press). Specimens were mounted and tested using a universal testing machine. A compressive load was applied at a 45° angle to the middle third of the palatal surface at a crosshead speed of 0.5 mm/min until failure occurred. Failure patterns were recorded and analyzed using SPSS software (version 13).

Results: Statistical analysis revealed no significant differences in the distribution of failure patterns between the two groups ($p > 0.05$, 95% confidence level).

Discussion: This study compared endocrowns and post-and-core restorations for endodontically treated maxillary central incisors. Both techniques showed comparable fracture resistance, with failure modes differing mainly in location and reparability. Endocrowns demonstrated favorable outcomes due to their minimally invasive design and improved stress distribution. These findings support endocrowns as a conservative alternative while confirming that both approaches can provide clinically acceptable performance.

Conclusion: Within the limitations of this *in vitro* study, endocrowns fabricated from lithium disilicate (IPS e.max Press) exhibited failure patterns comparable to those of the conventional technique involving quartz-fiber posts, composite cores, and lithium disilicate crowns when restoring severely compromised endodontically treated anterior teeth.

Keywords: Endocrowns, IPS e.max press, Endodontically treated anterior incisors, Quartz-fiber posts, Composite resin cores, Failure patterns.

© 2026 The Author(s). Published by Bentham Open.

This is an open access article distributed under the terms of the Creative Commons Attribution 4.0 International Public License (CC-BY 4.0), a copy of which is available at: <https://creativecommons.org/licenses/by/4.0/legalcode>. This license permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited.

*Address correspondence to this author at the Fixed Prosthodontics, Tishreen University, Latakia, Syrian Arab Republic; E-mail: abedalhade2223@gmail.com

Cite as: Kheder A, Saker R, Albash Z. Failure Patterns of Severely Compromised Endodontically Treated Anterior Teeth: A Comparative *In Vitro* Study of Two Restorative Approaches. Open Dent J, 2026; 20: e18742106440539. <http://dx.doi.org/10.2174/0118742106440539260407102718>



CrossMark

Received: September 18, 2025

Revised: December 06, 2025

Accepted: January 07, 2026

Published: April 27, 2026



Send Orders for Reprints to reprints@benthamscience.net

1. INTRODUCTION

Endodontically treated anterior teeth represent a considerable restorative challenge, largely due to the substantial loss of tooth structure that occurs following pulp treatment. This structural reduction adversely affects the resistance form of the tooth and, if not adequately managed, may increase susceptibility to fracture [1]. Conventionally, retention in such cases has been achieved through the use of intra-radicular post-and-core systems [2]. Although these restorations have been associated with acceptable clinical performance, their placement often requires the removal of additional radicular dentin, reported in some cases to exceed 50% in maxillary incisors, which may further weaken the remaining tooth structure and increase the risk of catastrophic root fractures [3, 4].

The clinical performance of post-and-core restorations is influenced by several interrelated factors, most notably the amount of remaining coronal tooth structure, root canal anatomy, and the mechanical properties of the post material [5]. Various post systems are currently available, including metallic posts, fiber-reinforced posts (such as glass, quartz, and carbon fibers), as well as newer materials like zirconia and PEEK [6]. Recent studies suggest that selecting a post material with a modulus of elasticity closer to that of dentin may contribute to more favorable stress distribution within the root structure, potentially reducing the risk of catastrophic failure [7].

Although conventional guidelines advocate a post length equivalent to two-thirds of the root and a diameter not exceeding one-third of the root width, the actual biomechanical significance of these recommendations remains a subject of ongoing debate [8]. As a more conservative restorative approach, endocrowns were introduced to reduce the need for extensive radicular preparation. Early designs consisted of amalgam coronal-radicular cores with limited extension into the root canal system [9].

The contemporary concept of the endocrown was later defined by Bindl and Mörmann in 1999, who described it as a bonded ceramic restoration that derives its primary retention from the pulp chamber rather than from post placement, with little to no extension into the root canals [10]. Currently, endocrowns can be fabricated from a range of adhesive materials, including lithium disilicate, leucite-reinforced and feldspathic ceramics, as well as resin-based composite materials [10]. With the advancement of adhesive dentistry, endocrowns have gained wide clinical acceptance for posterior teeth, particularly in situations involving short roots, calcified canals, or reduced occlusal clearance [10].

Their reported advantages include conservative dentin preservation, procedural simplification, and decreased chairside time. Nevertheless, the application of endocrowns in anterior teeth remains relatively limited, primarily due to the lack of long-term clinical evidence and persistent clinician concerns regarding esthetics and biomechanics [11].

Accordingly, the present study aimed to assess the biomechanical performance of endocrowns compared with

quartz fiber post-supported restorations in structurally compromised maxillary central incisors, to clarify the potential suitability of endocrowns for anterior applications.

1.1. Study Aim

The aim of this *in vitro* study was to evaluate and compare the failure patterns of lithium disilicate endocrowns used to restore severely compromised, endodontically treated maxillary central incisors with conventional lithium disilicate crowns supported by quartz fiber posts and composite resin cores.

2. MATERIALS AND METHODS

This study was approved by the Ethics Committee of the Faculty of Dentistry at Latakia University (approval No. 2379, dated 25-10-2021). It was conducted in accordance with the Declaration of Helsinki for human research [12].

2.1. Study Design

This study employed a randomized, controlled, and comparative *in vitro* experimental design.

Inclusion criteria: Recently extracted human maxillary central incisors with fully formed apices, single straight canals, no previous endodontic treatment, similar root dimensions (23 ± 1 mm), and intact roots free from cracks, caries, restorations, or resorption were included.

Exclusion criteria: Teeth with root caries, fractures, craze lines, internal or external resorption, calcified canals, curved roots, multiple canals, previous restorations, or structural anomalies were excluded from the study.

2.2. Sample Size Calculation

The required sample size was calculated using G*Power 3.1 software, assuming a 95% confidence level and a statistical power of 0.85. The study used a sample size of 20 specimens. Additionally, the tooth collection process was completed within 20 days.

2.3. Study Sample

The sample consisted of 20 recently extracted human maxillary central incisors obtained from patients who underwent extraction for periodontal reasons at the Faculty of Dentistry Clinics, Latakia University, Syria. Written informed consent was obtained from all patients for the use of extracted teeth for research purposes. All specimens were standardized in morphology and size (root length: 23 ± 1 mm; mesiodistal crown width: 7 ± 0.5 mm; buccolingual crown width: 9 ± 0.5 mm). After extraction, the teeth were thoroughly cleaned and stored in saline solution until testing. Once the sample was complete, the crown portion of each tooth was sectioned 2 mm above the Cemento-Enamel Junction (CEJ) using a straight handpiece and a 22-mm stainless steel laboratory separating disc [12].

All measurements and manual procedures, including preparation and cementation, were performed by a single operator (AK). Standardized root canal treatment was performed using a rotary endodontic system (Eighteenth E-Connect endo motor, Changzhou Sifary, China). Obturation was carried out with gutta-percha and an eugenol-free sealer. The specimens were then embedded in acrylic molds

of uniform dimensions and randomly assigned to two equal groups ($n = 10$): Group I (Endocrowns), restored with lithium disilicate endocrowns (IPS e.max Press), numbered 1-10, and Group II (Post-and-Core Crowns), restored with quartz-fiber posts and composite resin cores, followed by lithium disilicate crowns (IPS e.max Press), numbered 11-20 [12].

2.4. Tooth Preparation

2.4.1. Group I (Endocrowns)

Excess gutta-percha at the entrance of the pulp chamber was removed carefully. The pulp chamber floor was prepared to a depth of 3 mm into the root canal while maintaining at least 1 mm of surrounding dentin. A 2-mm ferrule was established, along with a 1-mm circumferential finish line at the CEJ (Fig. 1).

2.4.2. Preparation of Group II Teeth

The specimens in this group were prepared to receive full-coverage lithium disilicate ceramic crowns (IPS e.max Press). Tooth preparation was performed under continuous water cooling using a round-ended tapered diamond bur (DiAMANT, Germany, 199X016 FG) to obtain a uniform 2-mm coronal ferrule and a 1-mm circumferential finish line at the cemento-enamel junction (CEJ). The diamond bur was replaced after every three preparations to maintain cutting efficiency. The finish-line width was verified using a calibrated periodontal probe [12].

A specific drill was used to prepare the post space to a depth of 8 mm inside the canal, corresponding to a post diameter of 1.4 mm, while maintaining 4-5 mm of apical

gutta-percha. Subsequently, Quartz fiber posts (Quartz Fiber Resin Post, RTT, China) were cemented according to standard protocols. The canals were irrigated with 5.25% sodium hypochlorite (Canox, Syria), dried with oil-free air, and luted with a dual-cure self-adhesive resin cement (Breeze, Lot 8725242, Pentron, USA) following the manufacturer's instructions. Cement was applied to the post, which was then placed inside the canal, and excess cement was removed using a microbrush. Light curing was performed from the buccal, palatal, and incisal aspects with an LED curing unit (Light Curing LED, Medical Hema, China) at an intensity exceeding 1000 mW/cm² for 60 seconds [12].

2.5. Composite Core Build-up

The coronal portion of each specimen was rebuilt using a composite resin core. Dentin was etched with 37% phosphoric acid (Eco-Etch, Ivoclar Vivadent, Liechtenstein) for 15 seconds, rinsed, and dried with oil-free air. A universal bonding agent (Tetric N-Bond Universal, Ivoclar Vivadent, Liechtenstein) was applied and light-cured for 15 seconds. The core was built incrementally using a nanohybrid composite (Tetric N-Ceram, Lot 23503, Ivoclar Vivadent, Liechtenstein), with each layer not exceeding 1.5-2 mm in thickness. Each increment was light-cured individually for 40 seconds using the same LED curing unit. After completing the core build-up (Fig. 2A), the preparation was refined using a round-ended tapered diamond bur to remove undercuts and ensure smooth continuity between the composite core and natural tooth structure (Fig. 2B and C) [12].

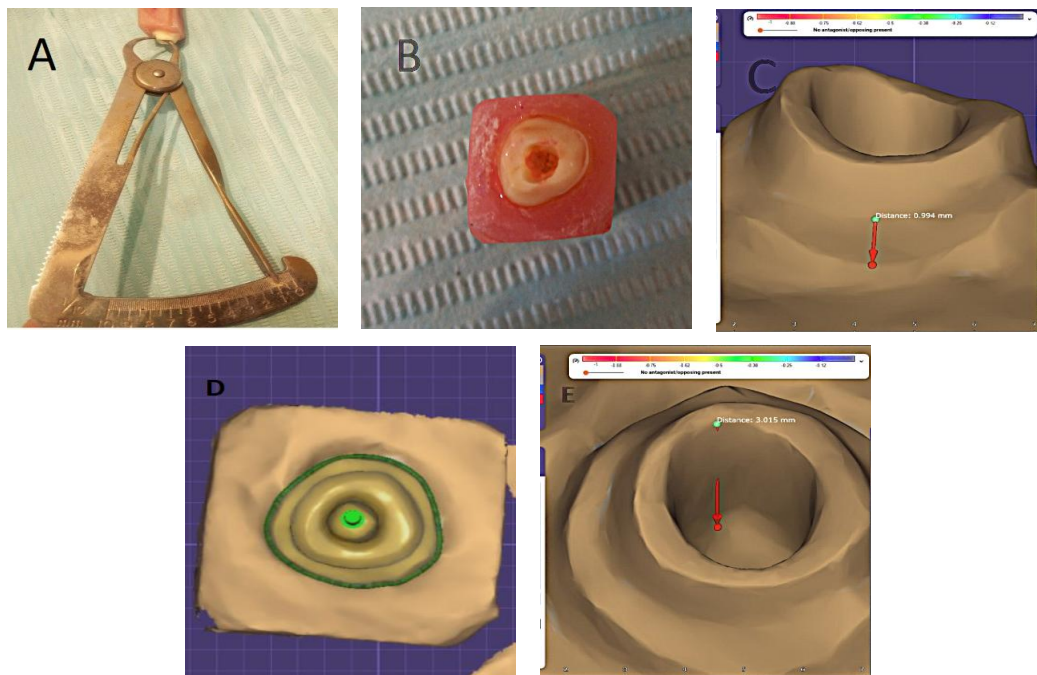


Fig. (1). **A)** The remaining dentin thickness around the preparation in one of the abutments from group one. **B)** Occlusal view of the preparation in one of the abutments from group on. **C)** Display of the finish line in one of the abutments from group one after scanning with the milling scanner. **D)** Occlusal view after scanning. **E)** Measurement of the preparation depth inside the pulp canal after scanning.

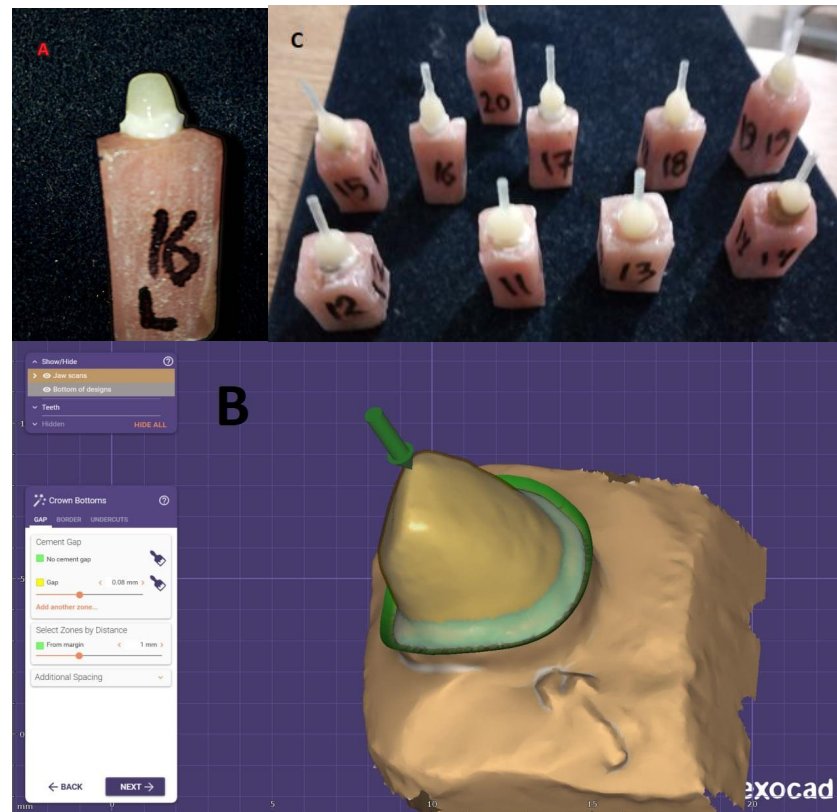


Fig. (2). **A)** One of the abutments from group two. **B)** Occlusal view and measurement of the finish line width of one of the abutments from Group Two after scanning with the optical scanner. **C)** Specimens of Group II.

2.6. Standardized Tooth Dimensions in Group II (Fig. 3)

All prepared teeth in this group were standardized according to the following parameters: Ferrule height: 2 mm; finish line width: 1 mm; core height (from finish line to incisal edge): 7 mm; maximum mesiodistal core width: 7 mm; maximum buccolingual core width: 5 mm [12]; and impression and model fabrication.

After tooth preparation in both experimental groups, impressions were obtained using plastic stock trays and the double-mix, single-step technique with condensation silicone (Zetaplus Putty and Oranwash L Light Body, Zhermack, Italy). Casts were poured using type IV dental stone (Marmorock, Siladent, Germany) and transferred to the laboratory. All specimens were stored in saline for 3 days before laboratory procedures were performed [12].

Stone casts were scanned using a DGSHAPE scanner, and three-dimensional digital models were processed using CAD software (exocad DentalDB, version 2016). Standardized wax patterns were designed with the following dimensions (Fig. 3): Incisogingival height (from finish line): 10.5 mm; maximum mesiodistal width: 9.2 mm; and maximum buccolingual width: 7 mm.

A 40- μ m cement space was applied between the restoration and tooth walls. Wax discs (VeriCORE Mill Wax) were milled using a 5-axis dry milling unit

(ROLAND® DGSHAPE DWX-52DCI) to produce standardized wax patterns with a 40- μ m cement space. Margins were sealed with casting wax (Renfert), and 3-mm wax sprues (Renfert) were attached following the manufacturer's recommendations (Fig. 4).

2.7. Pressing and Finishing Procedures

The wax patterns were invested and processed using IPS Press Vest (Ivoclar Vivadent). Pressing was performed in a ceramic press furnace following the manufacturer's protocol. The resulting restorations were conditioned with <1% hydrofluoric acid for 20 minutes, sandblasted with rubberized abrasive particles, rinsed, dried, and glazed according to the manufacturer's instructions, producing restorations ready for cementation [12].

2.8. Cementation

The internal and marginal fit of each ceramic restoration was verified prior to cementation. Restorations were cleaned with alcohol, rinsed with water, and air-dried. The intaglio surface, including the intracanal extension, was etched with 9.5% hydrofluoric acid (Porcelain Etchant 9.5%, Lot 220005167, Bisco, USA) for 90 seconds, rinsed thoroughly for 1 minute, and air-dried. Two layers of silane coupling agent (Porcelain Primer, Lot 220004029, Bisco, USA) were applied and allowed to react for 1 minute [12].

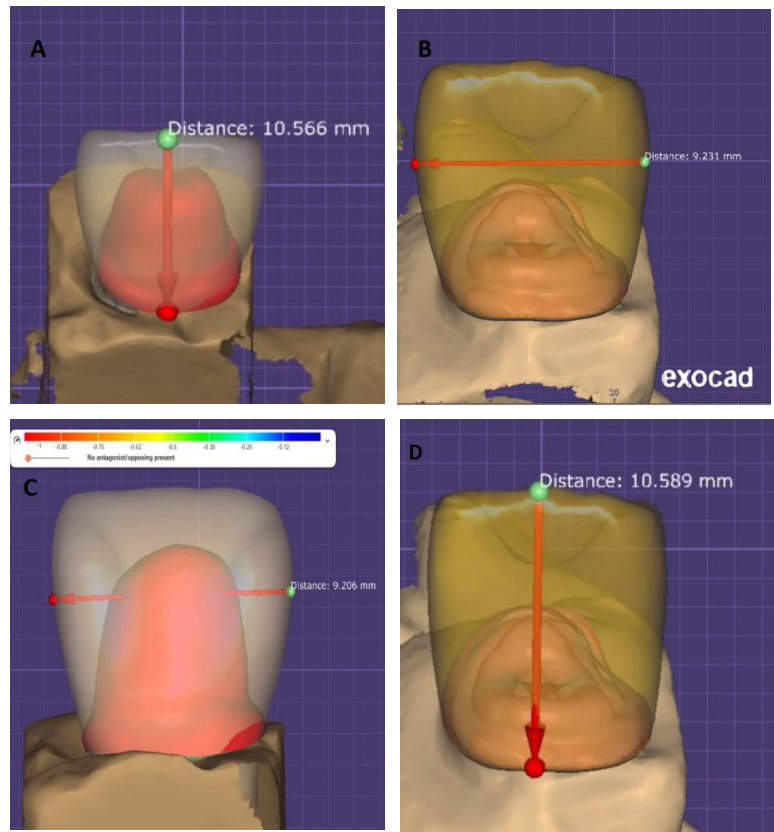


Fig. (3A-D). The measurements of the wax models before milling.

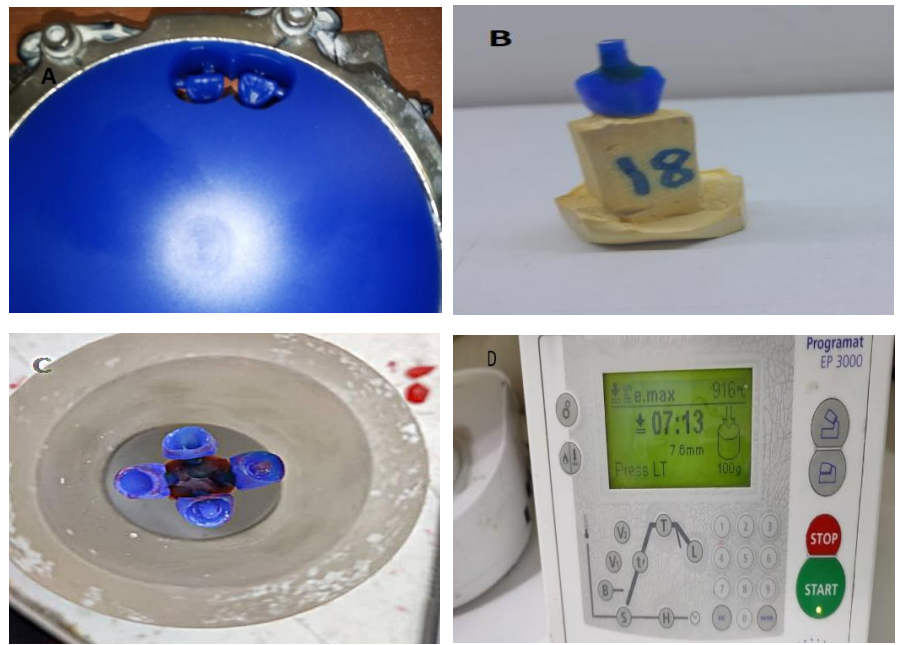


Fig. (4). A) Wax disc milling. B) Wax model anchoring. C) Final waxing with pins on the injection crucible base. D) Setting up the thermal injection device.

On the tooth surface, preparations were cleaned with pumice powder and a brush, rinsed, and dried. Enamel and dentin were etched with 37% phosphoric acid (Lot T38390, Ivoclar Vivadent, Liechtenstein) for 15 seconds, rinsed thoroughly, and air-dried for 20 seconds. A universal bonding agent (Tetric N-Bond Universal, W08416, Ivoclar Vivadent, Liechtenstein) was then applied, gently air-thinned, and light-cured for 20 seconds [12].

A dual-cure resin cement (MetaCem, Meta Biomed, Germany) was mixed according to the manufacturer's

instructions and applied to the internal surface of each restoration. Restorations were seated with light finger pressure, and excess cement was removed. Light curing was performed on the buccal, lingual, mesial, and distal aspects for 40 seconds per surface using the same LED curing unit (Fig. 5).

All specimens were stored in physiological saline solution for 48 hours before mechanical testing (Fig. 6A-C). A comparison between the two groups is presented in Fig. (7).

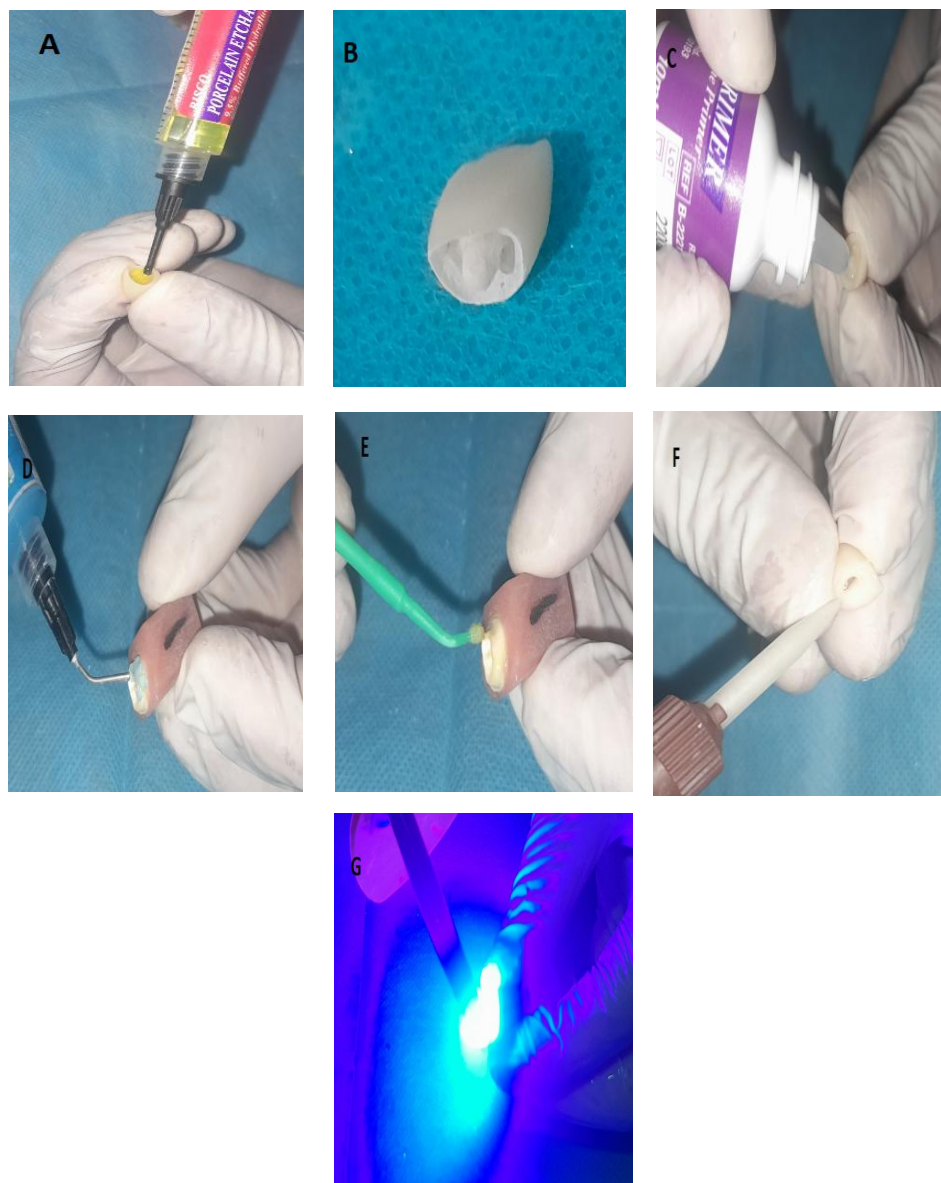


Fig. (5). **A)** Etching the internal surfaces of the restorations with 9.5% hydrofluoric acid. **B)** The chalky appearance of the porcelain after etching. **C)** Application of the dual bond agent (silane). **D)** Etching the abutments with 37% phosphoric acid. **E)** Applying bond. **F)** Application of the dual-cure resin cement. **G)** Curing the cement using a light-curing device.

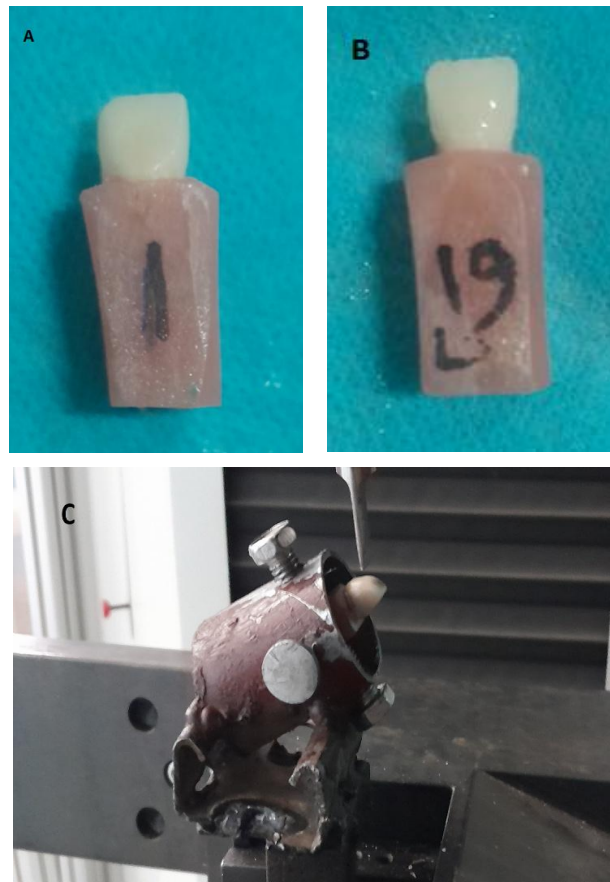


Fig. (6). (A and B) The final restoration after bonding. C) Applying oblique forces to the teeth at a 45-degree angle on a custom-made base.

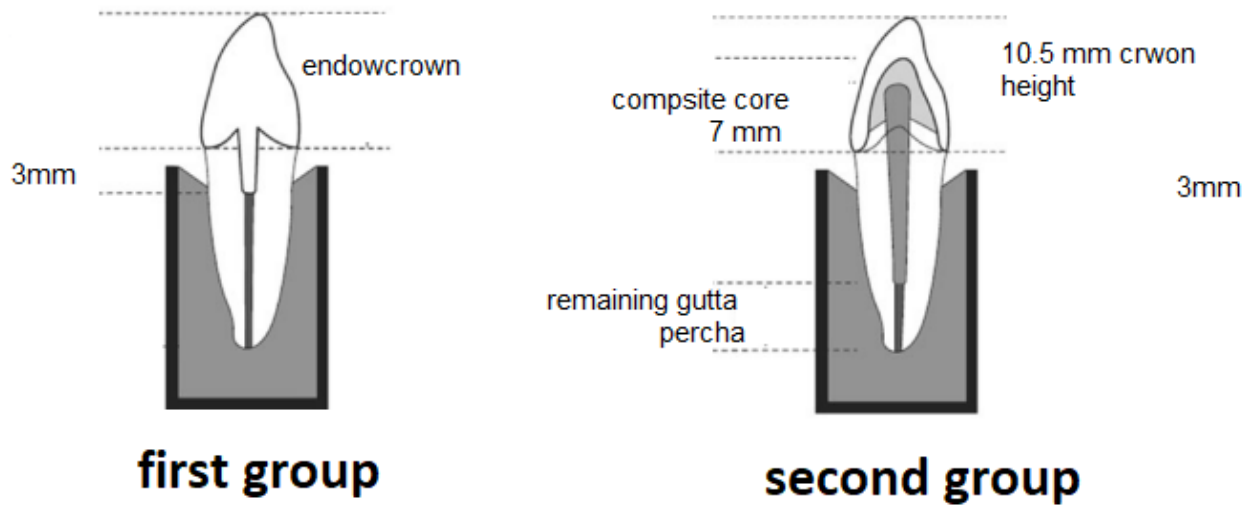


Fig. (7). Illustrates the final compound for both study groups.

2.9. Mechanical Testing

For fracture testing, each specimen was mounted in a custom-made base at a 45° angle to simulate functional loading. A knife-edge steel indenter (4-mm width) was positioned against the middle third of the palatal surface, and compressive loading was applied at a crosshead speed of 0.5 mm/min using a universal testing machine until failure occurred (Fig. 6C). Failure patterns were visually inspected (Fig. 7) and classified according to the categories used for the two experimental groups (Table 1). Statistical analysis was performed using SPSS software (version 13.1).

3. RESULTS

3.1. Sample Description

The study sample consisted of 20 extracted human maxillary central incisors with intact roots, standardized in length and morphology. The specimens were randomly divided into two equal groups (n = 10) according to the restorative technique, such as Group I consisting of lithium disilicate endocrowns (IPS e.max Press) extending 3 mm into the canal, and Group II comprising quartz-fiber posts and composite resin cores, followed by lithium disilicate crowns (IPS e.max Press).

3.2. Fracture Patterns

Fracture patterns were evaluated based on the visual assessment of each specimen after mechanical testing.

The following patterns were identified: Fracture of the restoration and tooth below the CEJ (Fig 8A and B); fracture of the restoration and tooth above the CEJ (Fig. 8C and D); fracture of the tooth below the CEJ (Fig. 8E); fracture of the restoration only (Fig. 8F and G); and debonding of the restoration (Fig. 8H).

Table 1 summarizes the distribution of fracture patterns according to the restorative technique.

3.3. Effect of Restorative Technique on Fracture Patterns

A Chi-square test was conducted to determine whether a statistically significant relationship existed between restorative technique and fracture pattern distribution, with Group I comprising lithium disilicate endocrowns (3-mm intracanal extension) and Group II consisting of quartz-fiber posts with composite resin cores and lithium disilicate crowns.

Table 2 presents the Chi-square analysis.

The p-value exceeded 0.05, indicating that no statistically significant differences were found between the two groups at the 95% confidence level regarding fracture pattern distribution.

3.4. Fracture Nature Assessment

Fractures were further classified as favorable or unfavorable based on their clinical reparability. The distribution of fracture types relative to restorative technique is illustrated in Fig. (9).

Table 1. Failure patterns observed in both groups.

Restorative Technique	Number of incisors						Percentage (%)					
	Fracture of the restoration and tooth below the (CEJ).	Fracture of the restoration and tooth above the (CEJ).	Fracture of the Tooth below the (CEJ).	Fracture of the Restoration only.	Debonding of the Restoration.	Total	Fracture of the Restoration and Tooth below the (CEJ).	Fracture of the restoration and tooth above the (CEJ).	Fracture of the Tooth below the (CEJ).	Fracture of the Restoration only.	Debonding of the Restoration.	Total
Endocrown restoration made of IPS e.max press extending 3 mm into the root canal	3	3	1	3	0	10	30.0	30.0	10.0	30.0	0	100
Quartz-fiber post with composite core and IPS e.max press crown	2	0	0	7	1	10	20.0	0	0	70.0	10.0	100
Total sample	5	3	1	10	1	20	25.0	15.0	5.0	50.0	5.0	100

Table 2. Results of the chi-square analysis.

The Studied variables = Fracture pattern × Restorative technique used				
Number of incisors (n)	Chi-square (χ²)	Degrees of freedom	p-value (Significance level)	Significance of differences
20	6.8	4	0.147	No statistically significant differences

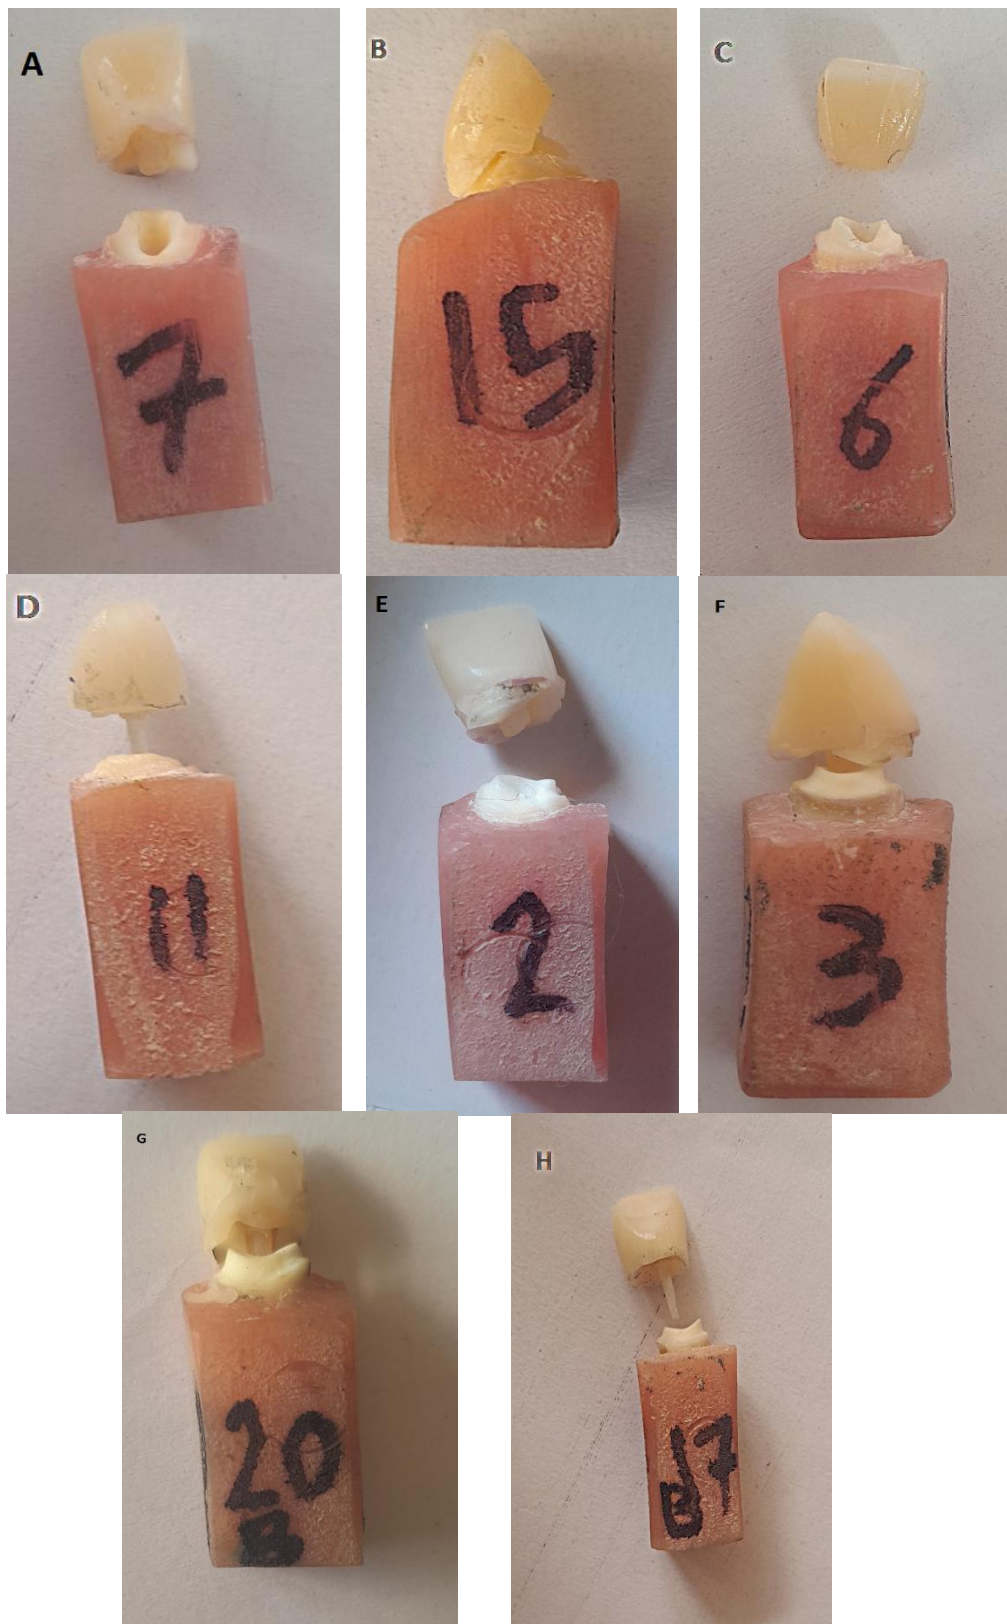


Fig. (8). (A and B) Fracture of the restoration and tooth below the CEJ. (C and D) Fracture of the restoration and tooth above the CEJ. (E) Fracture of the tooth below the CEJ. (F and G) Fracture of the restoration only. (H) Debonding of the restoration.

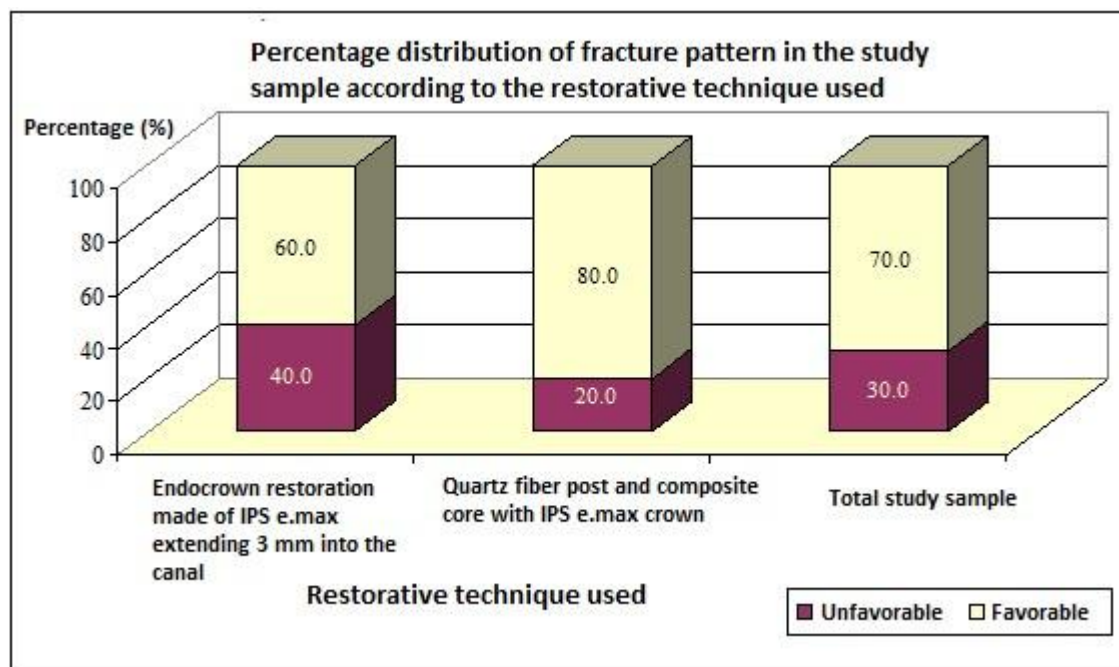


Fig. (9). Percentage distribution of the results of the nature of fractures in the study sample according to the restorative technique used.

Table 3. The outcomes of the chi-square test.

The Studied variables = Nature of fracture × Restorative technique used				
Number of incisors	Chi-square value	Degrees of freedom	Significance level (p-value)	Significance of differences
20	6.8	4	0.147	Not significant (NS)

3.5. Effect of Restorative Technique on Fracture Nature

The effect of restorative technique on fracture type was evaluated using a Chi-square test to determine whether the choice of technique influenced the nature of fractures, with Group I consisting of lithium disilicate endocrowns (3-mm intracanal extension) and Group II comprising quartz-fiber posts with composite cores and lithium disilicate crowns.

Results are summarized in Table 3, presenting the statistical comparison of favorable and unfavorable fracture types between groups.

3.6. Interpretation of Results

The obtained *p*-value was considerably greater than 0.05. This indicates that, at the 95% confidence level, there was no statistically significant difference in the distribution of fracture nature (favorable vs. unfavorable) between the two restorative approaches: lithium disilicate endocrowns (IPS e.max Press) with a 3 mm intracanal extension and quartz fiber-reinforced resin posts with composite cores and lithium disilicate crowns (IPS e.max Press).

4. DISCUSSION

This study evaluated two restorative approaches for structurally compromised, endodontically treated maxillary central incisors: (1) endocrowns fabricated from IPS e.max ceramic with a 3 mm intracanal extension, and (2) quartz fiber-reinforced resin posts with composite cores and IPS e.max crowns. The specimens were carefully selected to ensure similarity in morphology and dimensions, which resemble the clinical biomechanical conditions. The specimens were stored in saline for 20 days before testing, thus not affecting mechanical properties such as hardness [13].

Maxillary central incisors were chosen for their significant esthetic and functional importance. In addition, there is a limited number of studies evaluating endocrown restorations in anterior teeth [7]. Traditional post-and-core techniques often require the removal of significant amounts of sound tooth structure and may be a challenge during endodontic retreatment, especially in single-rooted teeth, in which post removal increases the risk of root fracture [14]. Furthermore, teeth with limited vertical dimension may prevent the usage of conventional posts and crowns [15], supporting the investigation of endocrowns as a more conservative restorative alternative.

Endocrowns are widely recognized for their minimally invasive design, reduced chairside time, and favorable esthetic outcomes. In addition, they provide a stable coronal seal that may limit bacterial microleakage, leading to improve the long-term prognosis of endodontically treated teeth. Another advantage of endocrowns is that retreatment is generally less complex compared with conventional post-and-core systems. Furthermore, several studies have reported that endocrowns show higher stability and fracture resistance, along with reducing the catastrophic root fractures [16].

A 3 mm intracanal extension was selected for the endocrown group, aligned with previous findings suggesting no significant differences in fracture resistance between 3 mm and 6 mm extensions in IPS e.max endocrowns [17]. In the post-and-core group, canal preparation extended to two-thirds of the root length (approximately 8 mm) [18], following established recommendations. IPS e.max was chosen due to its excellent mechanical properties and esthetic advantages [19], and composite core dimensions adhered strictly to the manufacturer's guidelines.

A standardized 1-mm finish line was prepared on both groups to ensure uniform stress distribution. CAD/CAM technology was used for designing and milling the wax patterns to ensure the accuracy of restoration fabrication [20].

The teeth were embedded in acrylic resin blocks to simulate clinical circumstances with a modulus of elasticity similar to that of natural bone [21]. Periodontal ligament simulation was ignored, aligning with studies showing its limited influence on fracture resistance outcomes [21].

The results revealed no statistically significant differences in the distribution of failure modes between the two restorative approaches. In the post-and-core group, failure was most frequently limited to the restoration itself, which can be attributed to the elastic modulus of quartz fiber posts (45–49 GPa) being closer to dentin (14–18 GPa) [22]. This biomechanical compatibility allows the post to flex under load, reducing stress concentration in the root and lowering the risk of catastrophic fractures. These observations are consistent with Sebastià *et al.* [23] and Zhou and Wang (2013) [24]. Stress distribution along the root in fiber post restorations explains why coronal restorative fractures predominated in this group [25].

Conversely, failure modes in the endocrown group were more heterogeneous, with one case of tooth fracture below the Cemento-Enamel Junction (CEJ). This could be explained by the strong micromechanical bonding of lithium disilicate ceramics with dental tissues, along with the reduced number of adhesive interfaces. Furthermore, the absence of an intraradicular post transfers functional stresses coronally, thereby localizing most failures at the restoration level rather than within the root.

Failure modes were categorized as favorable (restoration fracture, debonding, or fracture above the

CEJ) or unfavorable (fracture below the CEJ). Favorable failure patterns occurred in 80% of group I specimens and 60% of group II specimens, although the difference was not statistically significant. Interestingly, repairable failures appeared more frequently in the post-and-core group. This may be due to the monoblock-like integration of the endocrown with the tooth structure and the involvement of the root in intracanal fractures associated with the 3 mm extension.

These findings are consistent with the outcomes of Al Fodeh *et al.* (2023) [26] and Guo *et al.* (2016) [27], both of which reported no significant differences in the frequency of favorable failure modes between endocrowns and fiber-post-supported ceramic crowns. Our results also align with those of Bankoğlu Güngör *et al.* (2017) [28], who reported that lithium disilicate endocrowns more often led to tooth fractures, whereas fiber-post restorations tended to fail at the restoration level. However, their study did not classify failure modes as favorable or unfavorable. Also, Chang *et al.* (2009) [29] found no significant differences between endocrowns and glass fiber post-supported crowns, noticing that unfavorable failures predominated in both groups. This discrepancy may be attributed to methodological differences, including the use of leucite-reinforced ceramics, CEREC CAD/CAM systems, and axial loading protocols.

In contrast, our results differ from those reported by Pedrollo *et al.* (2017) [30], who observed no favorable failure patterns in the endocrown group, whereas 37.5% favorable failures were recorded in the fiber-post group. This discrepancy may be attributed to differences in study design. In their investigation, endocrowns featured a 5 mm intracanal extension, which could have adversely affected root integrity, and no cervical ferrule was prepared in the post-and-core group. Conversely, our protocol included a 2 mm ferrule, a design feature known to improve fracture resistance and decrease the unfavorable root fractures [31]. Additionally, methodological variations, such as their use of mandibular premolars and the application of 1,200,000 cyclic loading cycles prior to fracture testing, may have further contributed to the observed differences in outcomes.

Moving beyond the descriptive comparison of failure patterns, it is important to consider the biomechanical factors that may explain how the two restorative systems respond to oblique loading. In the endocrown group, retention is achieved through a single, continuous adhesive interface between the lithium disilicate restoration and the prepared cavity walls. This simplified bonding configuration limits the number of potential weak interfaces and may improve stress distribution. In addition, micromechanical retention is enhanced by hydrofluoric acid etching and silane application, which contribute to a more stable adhesive bond.

Previous studies have demonstrated that etched lithium disilicate forms a durable hybrid layer with resin cement. This strong bond improves the cohesive integrity of the tooth-restoration complex [32, 33]. As a result, failures in endocrowns tend to occur within the ceramic or

the underlying tooth structure rather than at the adhesive interface. This pattern is consistent with the mixed failure modes observed in the present study.

However, this strong adhesion also has biomechanical consequences. Because lithium disilicate has a high elastic modulus (~95 GPa), stresses generated under oblique loading tend to concentrate at the cervical margins and along the internal walls of the pulp chamber. Finite element analyses have shown that endocrowns can promote tensile stress accumulation in the cervical dentin. This effect is mainly related to the rigidity of the ceramic and its limited ability to absorb deformation, especially when intracanal extensions are present [34, 35].

In contrast, the post-and-core system incorporates multiple adhesive interfaces (dentin-cement, cement-fiber post, composite core-tooth, core-crown), each of which can act as a potential stress-attenuating interface. The quartz fiber post, with an elastic modulus closer to that of dentin (~45–50 GPa), promotes more favorable stress distribution along the root. This elastic compatibility reduces stress concentration in apical and cervical regions and redirects deformation coronally, making restoration-level fractures more common and root-level fractures less frequent [36, 37]. Additionally, the composite resin core acts as a stress-dissipating layer, limiting crack propagation toward the radicular dentin and supporting the prevalence of repairable coronal fractures [38].

Several investigations have shown that endocrowns tend to concentrate higher stresses in the cervical dentin. In contrast, fiber-post restorations demonstrate a more uniform stress distribution, largely due to the similarity between the elastic modulus of the post and that of natural dentin [35, 39]. These biomechanical differences may help explain the distinct failure tendencies observed between the two groups, even though no statistically significant difference in overall failure pattern distribution was detected in the present study.

5. STUDY LIMITATIONS

This *in vitro* study may not fully replicate the complexities of the oral environment, including variable loading patterns and thermal fluctuations. The relatively small sample size may limit the generalizability of the findings. Additionally, periodontal ligament simulation and long-term fatigue loading were not performed, which may have influenced the clinical relevance and applicability of the results.

CONCLUSION

No statistically significant differences were observed in the failure patterns between lithium disilicate endocrowns and quartz fiber post-composite core-supported lithium disilicate crowns used to restore structurally compromised, endodontically treated anterior teeth.

Within the limitations of this *in vitro* study, both restorative techniques demonstrated comparable mechanical performance.

The endocrown design may represent a more conservative restorative alternative; however, its clinical applicability warrants further investigation.

Future long-term clinical and laboratory studies incorporating fatigue loading and thermocycling protocols are recommended to better simulate intraoral conditions.

AUTHORS' CONTRIBUTIONS

The authors confirm contribution to the paper as follows: A.K., R.S.: Study conception and design; A.K., R.S.: Data collection; A.K., R.S.: Analysis and interpretation of results; A.K., R.S., Z.A.: Draft manuscript. All authors reviewed the results and approved the final version of the manuscript.

LIST OF ABBREVIATIONS

CEJ	= Cemento-Enamel Junction
CAD/CAM	= Computer-Aided Design / Computer-Aided Manufacturing
IPS e.max Press	= Ivoclar Pressed Lithium Disilicate Ceramic
PEEK	= Polyetheretherketone
SPSS	= Statistical Package for the Social Sciences
LED	= Light Emitting Diode
HF	= Hydrofluoric Acid
NaOCl	= Sodium Hypochlorite
Gpa	= Gigapascal
mm	= Millimeter
µm	= Micrometer
Mpa	= Megapascal
<i>p</i> -value	= Probability value
SD	= Standard Deviation
CI	= Confidence Interval
CEREC	= Chairside Economical Restoration of Esthetic Ceramics
E.max	= Lithium Disilicate Ceramic System
N	= Newton

ETHICS APPROVAL AND CONSENT TO PARTICIPATE

This study was approved by the Ethics Committee of the Faculty of Dentistry at Latakia University, Syrian Arab Republic (approval No. 2379, dated 25-10-2021).

HUMAN AND ANIMAL RIGHTS

All procedures performed in studies involving human participants were in accordance with the ethical standards of institutional and/or research committee and with the 1975 Declaration of Helsinki, as revised in 2013.

CONSENT FOR PUBLICATION

Informed consent was obtained from the participants.

AVAILABILITY OF DATA AND MATERIALS

The data and supportive information are available within the article.

FUNDING

None.

CONFLICT OF INTEREST

The authors declare no conflict of interest, financial or otherwise.

ACKNOWLEDGEMENTS

Declared none.

REFERENCES

- [1] Caussin E, Izart M, Ceinos R, Attal JP, Beres F, François P. Advanced material strategy for restoring damaged endodontically treated teeth: A comprehensive review. *Materials* 2024; 17(15): 3736. <http://dx.doi.org/10.3390/ma17153736> PMID: 39124400
- [2] Ak Korkut ŞS, Cimilli H. Restorations of endodontically treated teeth. *Selcuk Dental Journal* 2024; 11(1): 86-9. <http://dx.doi.org/10.15311/selcukdentj.1250382>
- [3] Lazari PC, Oliveira RCN, Anchieta RB, *et al.* Stress distribution on dentin-cement-post interface varying root canal and glass fiber post diameters. A three-dimensional finite element analysis based on micro-CT data. *J Appl Oral Sci* 2013; 21(6): 511-7. <http://dx.doi.org/10.1590/1679-775720130203> PMID: 24473716
- [4] Patel SR, Youngson C, Jarad F. Principles guiding the restoration of the root-filled tooth. *Br Dent J* 2025; 238(7): 508-16. <http://dx.doi.org/10.1038/s41415-025-8401-4> PMID: 40217033
- [5] Huang M, Wang B, Zhang K, Yan X, Chen Z, Zhang X. Comparative analysis of stress distribution in residual roots with different canal morphologies: Evaluating CAD/CAM glass fiber and other post-core materials. *BMC Oral Health* 2024; 24(1): 337. <http://dx.doi.org/10.1186/s12903-024-04109-9> PMID: 38491485
- [6] Badami V, Ketineni H, Pb S, Akarapu S, Mittapalli SP, Khan A. Comparative evaluation of different post materials on stress distribution in endodontically treated teeth using the finite element analysis method: A systematic review. *Cureus* 2022; 14(9): e29753. <http://dx.doi.org/10.7759/cureus.29753> PMID: 36324349
- [7] Madfa AA. Effect of dental glass fiber posts on root stresses and fracture behavior of endodontically treated maxillary central incisors: A finite element analysis study. *Cureus* 2023; 15(8): e43056. <http://dx.doi.org/10.7759/cureus.43056> PMID: 37680412
- [8] de Moraes DC, Butler S, Santos MJMC. Current insights on fiber posts: A narrative review of laboratory and clinical studies. *Dent J* 2023; 11(10): 236. <http://dx.doi.org/10.3390/dj11100236> PMID: 37886921
- [9] Nayyar A, Walton RE, Leonard LA. An amalgam coronal-radicular dowel and core technique for endodontically treated posterior teeth. *J Prosthet Dent* 1980; 43(5): 511-5. [http://dx.doi.org/10.1016/0022-3913\(80\)90322-4](http://dx.doi.org/10.1016/0022-3913(80)90322-4) PMID: 6988579
- [10] Lenz U, Bacchi A, Della Bona A. Biomechanical performance of endocrown and core-crown restorations: A systematic review. *J Esthet Restor Dent* 2024; 36(2): 303-23. <http://dx.doi.org/10.1111/jerd.13119> PMID: 37571973
- [11] Mously HA, Naguib GH, Abougazia AO, Almabadi AA, Qutub OA, Hamed MT. Anterior endocrowns as an alternative to core crown restorations: A systematic review. *Int Dent J* 2025; 75(1): 59-74. <http://dx.doi.org/10.1016/j.identj.2024.07.1216> PMID: 39306490
- [12] Kheder AA, Saker RJ, Baherli NA, Albash Z. Fracture resistance in severely damaged central incisors restored with two-restoration techniques: An *in vitro* study. *Open Dent J* 2025; 19(1): e18742106369913. <http://dx.doi.org/10.2174/0118742106369913250218045152>
- [13] Kantoor P, Srivastava N, Rana V, Adlakha VK. Alterations in the mechanical properties of the extracted human teeth to be used as biological restorations on storing them in different storage media: An *in vitro* study. *Dent Traumatol* 2015; 31(4): 308-13. <http://dx.doi.org/10.1111/edt.12158> PMID: 25645513
- [14] Haupt F, Riggers I, Konietzschke F, Rödiger T. Effectiveness of different fiber post removal techniques and their influence on dentinal microcrack formation. *Clin Oral Investig* 2022; 26(4): 3679-85. <http://dx.doi.org/10.1007/s00784-021-04338-0> PMID: 34893941
- [15] AlDabeeb DS, Alakeel NS, Al jfshar RM, Alkhalid TK. Endocrowns: Indications, preparation techniques, and material selection. *Cureus* 2023; 15(12): e49947. <http://dx.doi.org/10.7759/cureus.49947> PMID: 38058523
- [16] Silva-Sousa AC, Moris ICM, Barbosa AFS, *et al.* Effect of restorative treatment with endocrown and ferrule on the mechanical behavior of anterior endodontically treated teeth: An *in vitro* analysis. *J Mech Behav Biomed Mater* 2020; 112: 104019. <http://dx.doi.org/10.1016/j.jmbbm.2020.104019> PMID: 32829166
- [17] Kanat-Ertürk B, Sarıdağ S, Kösele E, Helvacioğlu-Yiğit D, Avcu E, Yildiran-Avcu Y. Fracture strengths of endocrown restorations fabricated with different preparation depths and CAD/CAM materials. *Dent Mater J* 2018; 37(2): 256-65. <http://dx.doi.org/10.4012/dmj.2017-035> PMID: 29311428
- [18] Çelik Uzun N, Uşun A, Çelik D. Unveiled stress dynamics: The role of post length and repair materials in perforated tooth models: A finite element analysis study. *BMC Oral Health* 2025; 25(1): 646. <http://dx.doi.org/10.1186/s12903-025-05750-8> PMID: 40287656
- [19] Lindner S, Frasheri I, Hickel R, Crispin A, Kessler A. Retrospective clinical study on the performance and aesthetic outcome of pressed lithium disilicate restorations in posterior teeth up to 8.3 years. *Clin Oral Investig* 2023; 27(12): 7383-93. <http://dx.doi.org/10.1007/s00784-023-05328-0> PMID: 37870592
- [20] Kumar MS, Kumar R, Saini RS, Vyas R, Vaddamanu SK. A comparative analysis of the accuracy of crown fabricated from conventional wax patterns and CAD/CAM technology - Milling and 3D printing. *J Pharm Bioallied Sci* 2024; 16(Suppl. 4): S3821-3. http://dx.doi.org/10.4103/jpbs.jpbs_985_24 PMID: 39927009
- [21] Kern M, Douglas WH, Fechtig T, Strub JR, DeLong R. Fracture strength of all-porcelain, resinbonded bridges after testing in an artificial oral environment. *J Dent* 1993; 21(2): 117-21. [http://dx.doi.org/10.1016/0300-5712\(93\)90160-R](http://dx.doi.org/10.1016/0300-5712(93)90160-R) PMID: 8473592
- [22] Atash R, Arab M, Duterme H, Cetik S. Comparison of resistance to fracture between three types of permanent restorations subjected to shear force: An *in vitro* study. *J Indian Prosthodont Soc* 2017; 17(3): 239-49. http://dx.doi.org/10.4103/jips.jpips_24_17 PMID: 28936037
- [23] Ramírez-Sebastià A, Bortolotto T, Cattani-Lorente M, Giner L, Roig M, Krejci I. Adhesive restoration of anterior endodontically treated teeth: Influence of post length on fracture strength. *Clin Oral Investig* 2014; 18(2): 545-54. <http://dx.doi.org/10.1007/s00784-013-0978-3> PMID: 23604697
- [24] Zhou L, Wang Q. Comparison of fracture resistance between cast posts and fiber posts: A meta-analysis of literature. *J Endod* 2013; 39(1): 11-5. <http://dx.doi.org/10.1016/j.joen.2012.09.026> PMID: 23228250
- [25] Comba A, Baldi A, Saratti CM, *et al.* Could different direct restoration techniques affect interfacial gap and fracture resistance of endodontically treated anterior teeth? *Clin Oral Investig* 2021; 25(10): 5967-75. <http://dx.doi.org/10.1007/s00784-021-03902-y> PMID: 33860368
- [26] Al Fodeh RS, Al-Johi OS, Alibrahim AN, Al-Dwairi ZN, Al-Haj Husain N, Özcan M. Fracture strength of endocrown maxillary restorations using different preparation designs and materials. *J Mech Behav Biomed Mater* 2023; 148: 106184. <http://dx.doi.org/10.1016/j.jmbbm.2023.106184> PMID: 37839334
- [27] Guo J, Wang Z, Li X, Sun C, Gao E, Li H. A comparison of the fracture resistances of endodontically treated mandibular

- premolars restored with endocrowns and glass fiber post-core retained conventional crowns. *J Adv Prosthodont* 2016; 8(6): 489-93.
<http://dx.doi.org/10.4047/jap.2016.8.6.489> PMID: 28018567
- [28] Bankoğlu Güngör M, Turhan Bal B, Yilmaz H, Aydin C, Karakoca Nemli S. Fracture strength of CAD/CAM fabricated lithium disilicate and resin nano ceramic restorations used for endodontically treated teeth. *Dent Mater J* 2017; 36(2): 135-41.
<http://dx.doi.org/10.4012/dmj.2016-017> PMID: 28111383
- [29] Chang CY, Kuo JS, Lin YS, Chang YH. Fracture resistance and failure modes of CEREC endo-crowns and conventional post and core-supported CEREC crowns. *J Dent Sci* 2009; 4(3): 110-7.
[http://dx.doi.org/10.1016/S1991-7902\(09\)60016-7](http://dx.doi.org/10.1016/S1991-7902(09)60016-7)
- [30] Pedrollo Lise D, Van Ende A, De Munck J, Umeda Suzuki TY, Cardoso Vieira LC, Van Meerbeek B. Biomechanical behavior of endodontically treated premolars using different preparation designs and CAD/CAM materials. *J Dent* 2017; 59: 54-61.
<http://dx.doi.org/10.1016/j.jdent.2017.02.007> PMID: 28214537
- [31] Stankiewicz NR, Wilson PR. The ferrule effect: A literature review. *Int Endod J* 2002; 35(7): 575-81.
<http://dx.doi.org/10.1046/j.1365-2591.2002.00557.x> PMID: 12190896
- [32] Zarone F, Ferrari M, Mangano FG, Leone R, Sorrentino R. "Digitally Oriented Materials": Focus on lithium disilicate ceramics. *Int J Dent* 2016; 2016: 9840594.
<http://dx.doi.org/10.1155/2016/9840594> PMID: 27635140
- [33] Hooshmand T, Rostami G, Behroozibakhsh M, Fatemi M, Keshvad A, van Noort R. Interfacial fracture toughness of different resin cements bonded to a lithium disilicate glass ceramic. *J Dent* 2012; 40(2): 139-45.
<http://dx.doi.org/10.1016/j.jdent.2011.12.005> PMID: 22182467
- [34] Taha D, Spintzyk S, Schille C, *et al.* Fracture resistance and failure modes of polymer infiltrated ceramic endocrown restorations with variations in margin design and occlusal thickness. *J Prosthodont Res* 2018; 62(3): 293-7.
<http://dx.doi.org/10.1016/j.jpor.2017.11.003> PMID: 29241944
- [35] Tribst JPM, Dal Piva AMO, Madruga CFL, *et al.* Endocrown restorations: Influence of dental remnant and restorative material on stress distribution. *Dent Mater* 2018; 34(10): 1466-73.
<http://dx.doi.org/10.1016/j.dental.2018.06.012> PMID: 29935769
- [36] Plotino G, Grande NM, Bedini R, Pameijer CH, Somma F. Flexural properties of endodontic posts and human root dentin. *Dent Mater* 2007; 23(9): 1129-35.
<http://dx.doi.org/10.1016/j.dental.2006.06.047> PMID: 17116326
- [37] Naumann M, Schmitter M, Frankenberger R, Krastl G. "Ferrule Comes First. Post Is Second!" Fake news and alternative facts? A systematic review. *J Endod* 2018; 44(2): 212-9.
<http://dx.doi.org/10.1016/j.joen.2017.09.020> PMID: 29229457
- [38] Soares CJ, Santana FR, Silva NR, Preira JC, Pereira CA. Influence of the endodontic treatment on mechanical properties of root dentin. *J Endod* 2007; 33(5): 603-6.
<http://dx.doi.org/10.1016/j.joen.2007.01.016> PMID: 17437882
- [39] Ausiello P, Ciaramella S, Martorelli M, *et al.* Mechanical behavior of endodontically restored canine teeth: Effects of ferrule, post material and shape. *Dent Mater* 2017; 33(12): 1466-72.
<http://dx.doi.org/10.1016/j.dental.2017.10.009> PMID: 29126633

DISCLAIMER: The above article has been published, as is, ahead-of-print, to provide early visibility but is not the final version. Major publication processes like copyediting, proofing, typesetting and further review are still to be done and may lead to changes in the final published version, if it is eventually published. All legal disclaimers that apply to the final published article also apply to this ahead-of-print version.